



Surgical procedures



$$A = \pi (r_1 \times S_1 - r_2 \times S)$$



Connective
Contour



Contents

| | |
|---|----|
| Introduction | 4 |
| Drilling sequence overview | 5 |
| Drilling sequences | |
| OsseoSpeed™ TX 3.0 S | 6 |
| OsseoSpeed™ TX 3.5 S | 7 |
| OsseoSpeed™ TX 4.0 S | 8 |
| OsseoSpeed™ TX 4.0 S – 6 mm | 9 |
| OsseoSpeed™ TX 4.5 | 10 |
| OsseoSpeed™ TX 5.0 | 11 |
| OsseoSpeed™ TX 5.0 S | 12 |
| Implant surgery | 13 |
| Standard drilling protocol for | |
| OsseoSpeed™ TX 4.5 and 4.0 S | 14 |
| One- and two-stage procedures | 16 |
| Overview and considerations | 17 |
| Pre-operative procedures | 17 |
| – Pre-operative examination | 17 |
| – Pre-operative planning | 17 |
| – Implant-bone relationship | 18 |
| – Loading guidelines | 18 |
| – Surgical considerations | 18 |
| Implant overview | 19 |
| Drill overview | 20 |
| Preparation | 22 |
| Implant | 22 |
| Healing Abutment and Cover Screw | 23 |
| Surgical Tray and instruments | 24 |
| Cleaning and sterilization guidelines | 25 |
| References supporting Astra Tech Implant System™ | 26 |

This manual is designed for use by clinicians who have undergone at least basic surgical and in-clinic implant training. Staying current on the latest trends and treatment techniques in implant dentistry through continued education is the responsibility of the clinician.

Function, beauty and biology in perfect harmony

Our aim is to provide you with the freedom of unlimited possibilities when it comes to implant therapy. We develop products and solutions to help make your job as simple as possible but we never compromise when it comes to reliable long-term esthetics and function. We always respect the body's own healing processes and by our holistic approach to implant therapy, reflected in the Astra Tech BioManagement Complex™, the result is function, beauty and biology in perfect harmony.


The Astra Tech Implant System™:

- One system for all indications
- Suitable for both one-stage and two-stage surgery
- Designed for immediate and early loading
- One connection in three sizes
- Carrier-free implant installation
- Color-coded packaging



Drilling sequence overview OsseoSpeed™ TX

| Implants | Drilling protocol – soft bone | Drilling protocol – standard | Drilling protocol – dense bone |
|---|---|---|--|
|  <p>OsseoSpeed™ TX 3.0 S</p> |  |  |  |
|  <p>OsseoSpeed™ TX 3.5 S</p> |  |  |  |
|  <p>OsseoSpeed™ TX 4.0 S</p> |  |  |  |
|  <p>OsseoSpeed™ TX 4.5</p> |  |  |  |
|  <p>OsseoSpeed™ TX 5.0</p> |  |  |  |
|  <p>OsseoSpeed™ TX 5.0 S</p> |  |  |  |

 = Drill only through the cortical bone, should not be used to full depth



OsseoSpeed™ TX 3.0 S

Drilling protocol – STANDARD



| | | | |
|-------------|-----------------|-----------------|----------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 2.7 | OsseoSpeed™ TX 3.0 S 13 mm |
|-------------|-----------------|-----------------|----------------------------|

Optional drill



Pilot Drill is available as an optional step within the drilling sequence.

Ø 2.0/2.7 mm

Drilling protocol – SOFT BONE




| | | | |
|-------------|-----------------|-----------------|----------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 2.7 | OsseoSpeed™ TX 3.0 S 13 mm |
|-------------|-----------------|-----------------|----------------------------|

Drilling protocol – DENSE BONE



| | | | | | |
|-------------|-----------------|-----------------|------------------------|------------------|----------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 2.7 | Cortical Drill 2.7/3.0 | Twist Drill 2.85 | OsseoSpeed™ TX 3.0 S 13 mm |
|-------------|-----------------|-----------------|------------------------|------------------|----------------------------|

 = Drill only through the cortical bone, should not be used to full depth



OsseoSpeed™ TX 3.5 S

Drilling protocol – STANDARD



| | | | |
|----------------|-----------------------|-----------------------|----------------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | OsseoSpeed™ TX 3.5 S 13 mm |
|----------------|-----------------------|-----------------------|----------------------------------|

Optional drill



Pilot Drill is available as an optional step within the drilling sequence.

Ø 2.0/3.2 mm

Drilling protocol – SOFT BONE




| | | | | |
|----------------|-----------------------|-----------------------|-----------------------|----------------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 2.7 | Twist Drill 3.2 | OsseoSpeed™ TX 3.5 S 13 mm |
|----------------|-----------------------|-----------------------|-----------------------|----------------------------------|

Drilling protocol – DENSE BONE



| | | | | | |
|----------------|-----------------------|-----------------------|------------------------------|------------------------|----------------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Cortical Drill 3.2/3.5 | Twist Drill 3.35 | OsseoSpeed™ TX 3.5 S 13 mm |
|----------------|-----------------------|-----------------------|------------------------------|------------------------|----------------------------------|

 = Drill only through the cortical bone, should not be used to full depth



Drilling protocol – STANDARD



| | | | | |
|-------------|-----------------|-----------------|-----------------|----------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Twist Drill 3.7 | OsseoSpeed™ TX 4.0 S 13 mm |
|-------------|-----------------|-----------------|-----------------|----------------------------|

Optional drills



Pilot Drills are available as an optional step within the drilling sequence.

Ø 2.0/3.2 mm
Ø 3.2/3.7 mm

Drilling protocol – SOFT BONE



| | | | | |
|-------------|-----------------|-----------------|-----------------|----------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Twist Drill 3.7 | OsseoSpeed™ TX 4.0 S 13 mm |
|-------------|-----------------|-----------------|-----------------|----------------------------|

Drilling protocol – DENSE BONE



| | | | | | | |
|-------------|-----------------|-----------------|-----------------|------------------------|------------------|----------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Twist Drill 3.7 | Cortical Drill 3.7/4.0 | Twist Drill 3.85 | OsseoSpeed™ TX 4.0 S 13 mm |
|-------------|-----------------|-----------------|-----------------|------------------------|------------------|----------------------------|

 = Drill only through the cortical bone, should not be used to full depth

 OsseoSpeed™ TX 4.0 S – 6 mm

Drilling protocol – STANDARD



| | | | | |
|-------------|-----------------|-----------------|-----------------|---------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Twist Drill 3.7 | OsseoSpeed™ TX 4.0 S 6 mm |
|-------------|-----------------|-----------------|-----------------|---------------------------|


Optional drill



Pilot Drill is available as an optional step within the drilling sequence.

Ø 2.0/3.2 mm

Drilling protocol – SOFT BONE

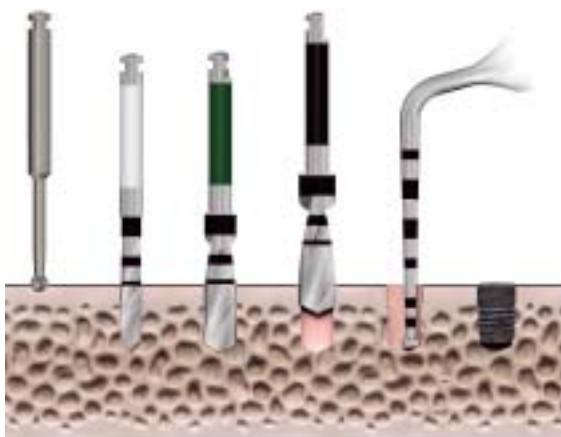


| | | | | |
|-------------|-----------------|-----------------|-----------------|---------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Twist Drill 3.7 | OsseoSpeed™ TX 4.0 S 6 mm |
|-------------|-----------------|-----------------|-----------------|---------------------------|

Drilling protocol – DENSE BONE



| | | | | | | |
|-------------|-----------------|-----------------|-----------------|------------------------|------------------|---------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Twist Drill 3.7 | Cortical Drill 3.7/4.0 | Twist Drill 3.85 | OsseoSpeed™ TX 4.0 S 6 mm |
|-------------|-----------------|-----------------|-----------------|------------------------|------------------|---------------------------|

 = Drill only through the cortical bone, should not be used to full depth



Drilling protocol – STANDARD



| | | | | |
|-------------|-----------------|-----------------|-----------------------|--------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Conical Drill 3.2/4.5 | OsseoSpeed™ TX 4.5 13 mm |
|-------------|-----------------|-----------------|-----------------------|--------------------------|

Optional drill



Pilot Drill is available as an optional step within the drilling sequence.

Ø 2.0/3.2 mm

Drilling protocol – SOFT BONE



| | | | | |
|-------------|-----------------|-----------------|-----------------------|--------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 2.7 | Conical Drill 2.7/4.5 | OsseoSpeed™ TX 4.5 13 mm |
|-------------|-----------------|-----------------|-----------------------|--------------------------|

Drilling protocol – DENSE BONE



| | | | | | |
|-------------|-----------------|-----------------|-----------------------|------------------|--------------------------|
| Guide Drill | Twist Drill 2.0 | Twist Drill 3.2 | Conical Drill 3.2/4.5 | Twist Drill 3.35 | OsseoSpeed™ TX 4.5 13 mm |
|-------------|-----------------|-----------------|-----------------------|------------------|--------------------------|



Drilling protocol – STANDARD



| | | | | | |
|-------------|-------------|-------------|-------------|---------------|----------------|
| Guide Drill | Twist Drill | Twist Drill | Twist Drill | Conical Drill | OsseoSpeed™ TX |
| | 2.0 | 3.2 | 3.7 | 3.7/5.0 | 5.0 |
| | | | | | 13 mm |

Optional drills



Pilot Drills are available as an optional step within the drilling sequence.

- Ø 2.0/3.2 mm
- Ø 3.2/3.7 mm

Drilling protocol – SOFT BONE



| | | | | |
|-------------|-------------|-------------|---------------|----------------|
| Guide Drill | Twist Drill | Twist Drill | Conical Drill | OsseoSpeed™ TX |
| | 2.0 | 3.2 | 3.2/5.0 | 5.0 |
| | | | | 13 mm |

Drilling protocol – DENSE BONE



| | | | | | | |
|-------------|-------------|-------------|-------------|---------------|-------------|----------------|
| Guide Drill | Twist Drill | Twist Drill | Twist Drill | Conical Drill | Twist Drill | OsseoSpeed™ TX |
| | 2.0 | 3.2 | 3.7 | 3.7/5.0 | 3.85 | 5.0 |
| | | | | | | 13 mm |

DRILLING SEQUENCES

OsseoSpeed™ TX 5.0 S



Drilling protocol – STANDARD



| | | | | | | |
|-------------|-------------|-------------|-------------|-------------|-------------|----------------|
| Guide Drill | Twist Drill | Twist Drill | Twist Drill | Twist Drill | Twist Drill | OsseoSpeed™ TX |
| | 2.0 | 3.2 | 3.7 | 4.2 | 4.7 | 5.0 S |
| | | | | | | 13 mm |


Optional drills



Pilot Drills are available as an optional step within the drilling sequence.

- Ø 2.0/3.2 mm
- Ø 3.2/3.7 mm
- Ø 3.7/4.2 mm

Drilling protocol – SOFT BONE

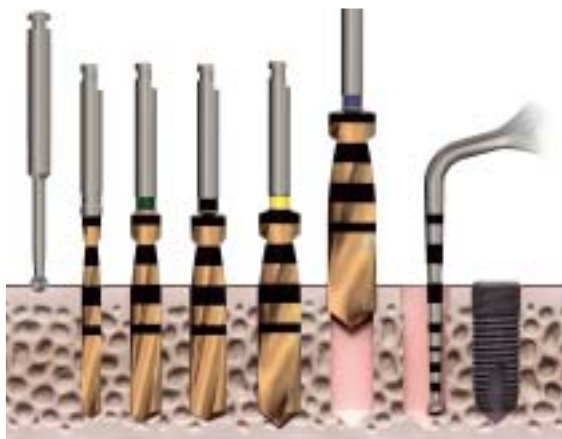

| | | | | | | |
|-------------|-------------|-------------|-------------|-------------|-------------|----------------|
| Guide Drill | Twist Drill | Twist Drill | Twist Drill | Twist Drill | Twist Drill | OsseoSpeed™ TX |
| | 2.0 | 3.2 | 3.7 | 4.2 | 4.7 | 5.0 S |
| | | | | | | 13 mm |

Drilling protocol – DENSE BONE



| | | | | | | | | |
|-------------|-------------|-------------|-------------|-------------|-------------|----------------|-------------|----------------|
| Guide Drill | Twist Drill | Twist Drill | Twist Drill | Twist Drill | Twist Drill | Cortical Drill | Twist Drill | OsseoSpeed™ TX |
| | 2.0 | 3.2 | 3.7 | 4.2 | 4.7 | 4.7/5.0 | 4.85 | 5.0 S |
| | | | | | | | | 13 mm |

 = Drill only through the cortical bone, should not be used to full depth

Implant installation – standard drilling protocol

Step-by-step procedures for placement of OsseoSpeed™ TX 4.5 and 4.0 S, 13 mm

Regardless of the pre-operative planning and choice of surgical protocol, the treatment with dental implants includes a site preparation and installation of the implant.

The following is an overview of an implant site preparation according to the standard drilling protocol for the installation of Astra Tech OsseoSpeed™ TX implants 4.5 and 4.0 S.

Note: All drilling should be performed at a speed of 1500 rpm and under profuse irrigation.



Guide Drill

Mark out the planned position of the implant site. This will also provide valuable information about the bone quality.

(Use of an acrylic stent shown here)



Twist Drill 2.0

Drill in the planned direction to the appropriate depth.

Note: Depth should allow implant to be level or slightly submerged in relation to adjacent marginal bone.

Place Direction Indicator in the site to facilitate the direction of the subsequent drilling.



Twist Drill 3.2

Drill the implant site to the appropriate depth.

IMPLANT SURGERY

Standard drilling protocol for a 4.5 and 4.0 S implant



Conical Drill 4.5

Finalize the osteotomy for the OsseoSpeed™ TX 4.5 implant, with the Conical Drill 4.5.

In standard and soft bone: drill to the beginning of the depth indication line.

In dense bone: drill to the full depth of the depth indication line.

Make sure there is enough depth provided for the entire implant. Sometimes additional drilling with a twist drill is needed. Always measure the depth using the Implant Depth Gauge.



Implant Depth Gauge

It is important to verify the drilling depth after the drilling with the Conical Drill is completed. Place the Depth Gauge against the wall of the osteotomy to verify the drilling depth.



Implant installation – OsseoSpeed™ TX 4.5

Install the implant with a contra angle at low speed (25 rpm) under profuse irrigation. Set the maximum torque to 35 Ncm. Let the implant work its way into the osteotomy and avoid applying unnecessary pressure.



Implant installation continue

The Ratchet Wrench, in combination with the Driver Handle, may be used for the final manual seating of the implant.

Use light finger force when leveling the implant. Excessive force with the Ratchet Wrench must be avoided as this will cause too much compression in the bone. A too high torque indicates that the implant needs to be retrieved for additional drilling.



Positioning the implant

Position the implant at the marginal bone level or slightly below. The objective is to get the implant in contact with as much cortical bone as possible.

Position one of the flat surfaces of the Implant Driver buccally to facilitate optimal placement of the chosen abutment. This especially applies to pre-designed abutments, such as TiDesign™ and ZirDesign™.

Release the Implant Driver from the implant by shifting it slightly from side to side.



Twist Drill 3.7 – for OsseoSpeed™ TX 4.0 S

Use a Twist Drill 3.7 to finalize the osteotomy for an OsseoSpeed™ TX 4.0 S implant.

Note: This sequence is not applicable for the 4.5 implant, where the final twist drill is 3.2 mm.



Implant installation – OsseoSpeed™ TX 4.0 S

Install the implant with a contra angle at low speed (25 rpm) under profuse irrigation. Set the maximum torque to 35 Ncm. Let the implant work its way into the osteotomy and avoid applying unnecessary pressure.

IMPLANT SURGERY
One- and two-stage procedures



One-stage procedure
Healing Abutment

Using light finger force (5–10 Ncm), seat the Healing Abutment.

Adapt and suture back the soft tissue flaps for a tight seal around the abutments.

They remain in place during the soft tissue healing phase and should then be replaced by permanent abutments.



One-stage procedure
Temporary or permanent abutment

Optional:

A one-stage surgical procedure may include a temporary prosthetic restoration attached to temporary or permanent abutments.



Two-stage procedure
Installation of Cover Screw

Insert the Cover Screw into the implant and tighten with only light finger force or with a contra angle preset at 25 rpm and 5–10 Ncm torque.

Reposition the mucoperiosteal flaps carefully and suture tightly together.



Two-stage procedure
Installation of abutment

After an appropriate healing phase the Cover Screw is exposed and removed using the Hex Screwdriver. Install the selected abutment into the implant.

For abutment selection and details, please refer to Cement-, Screw- or Attachment-retained manuals.

Pre-operative procedures

Pre-operative examination

The pre-operative examination should include a general evaluation of the patient's health and a clinical and oral radiographic examination. Particular attention should be given to mucous membranes, jaw morphology, dental and prosthetic history, and signs of dysfunction.

A radiographic analysis should be used to evaluate bone quality and the topography of the residual alveolar process. The initial radiographic evaluation, together with the clinical examination, is the basis for determining whether or not a patient is a candidate for implant treatment.

If the patient is found to be suitable, a more thorough clinical examination of the area for treatment and the opposing jaw should be performed. Any local pathology in the jaws should be treated before implant placement.

Pre-operative planning

Models from both jaws should be mounted on an articulator and the relationship between the alveolar ridges and teeth studied. A diagnostic wax-up, replacing the missing teeth, should be made on the model.

An analysis to evaluate the occlusal table, force distribution, and preferred sites for the implants should then be performed. When an optimal situation is achieved on the articulator, a duplicate model of the wax-up should be fabricated and an acrylic stent produced from this model. The stent should then be used during implant installation to guide the placement of the implants in terms of both position and inclination, taking into account anatomical, functional, esthetic, hygienic, and phonetic factors.


A transparent Radiographic Implant Guide, presenting implants in different magnifications, is helpful for planning optimal implant position and direction.

A Computer Guided Implant Treatment software such as Facilitate™ can also be helpful in order to ensure accurate planning for optimized implant position and placement. *For more information please refer to the Facilitate™ Procedures Manual.*

Even though the final treatment approach is usually not determined until the time of surgery the following should be considered based on the quality of supporting bone and initial stability of the implants:

- Whether a one- or two-stage surgical procedure will be preformed
- If an immediate or early loading protocol will be used
- What is the expected healing time before loading

Before treatment begins, the patient should be informed about the results of the pre-operative examination and given a clear explanation of what is entailed by the planned treatment, including the expected outcome and risks involved.

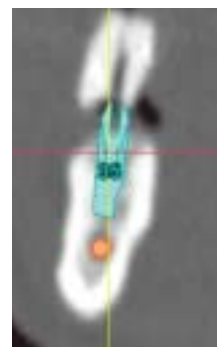

Implant-bone relationship

Factors influencing the implant-bone relationship are:

- Bone quantity
- Bone quality
- Diameter of the drilled implant site
- Depth of the drilled implant site

The implant site must be prepared in such a way that:

- The installed implant can achieve primary stability
- No harmful stress to the bone is induced during implant placement

Limited vertical dimension of bone for implant support may be compensated for by an increased implant diameter, provided that sufficient bone support around the implant is present. Optimal bone support can be additionally gained through the use of OsseoSpeed™ TX implants. The surgical methods, together with prosthetic flexibility for different implant positions, can often compensate for reduced bone quantity.

When bone quality and quantity are compromised, the utilization of osteotome techniques can help to improve the conditions for implant placement and the soft bone drilling protocol provides a perception of increased torque resistance during implant installation.



Loading guidelines

A three-month healing period in the mandible and a six-month healing period in the maxilla before loading were originally advocated for implants. Extensive research and product development have shown that reduced healing times can be applied which has been documented in numerous clinical studies. However, when a shorter healing time before loading is being considered, the assessment must always be based on the individual clinical situation.

Bone quality and quantity, design of superstructure, loading conditions, and primary stability achieved, should be carefully examined and assessed.

Immediate loading protocol may be utilized when:

- Good primary stability can be achieved
- There is no risk of traumatic loading
- A one-stage protocol can be recommended
- There is no need for grafting procedures in close relation to implant surgery

Early loading protocol

When the prerequisites for immediate loading cannot be met, an early loading protocol (six weeks or more healing period) may be considered. It is the responsibility of the clinician to determine which loading protocol to use based on each individual case.

Surgical considerations

Supported by Facilitate™ Computer Guided Surgery the implant installation is sometimes performed without flaps being raised. This reduced surgical intervention is reported to give less postoperative swelling and pain than the conventional surgical protocol with incision and flap elevation, however it must be stressed that there is no documentation available evaluating risks for surgical errors and other complications using this method. It is up to the discretion and responsibility of each individual clinician which surgical approach to choose.

Implant overview

The OsseoSpeed™ TX implants have been developed and extensively documented for both one- and two-stage surgical procedures.













Intended use

- In replacing missing teeth in single or multiple unit applications within the mandible or maxilla
- Indicated for immediate placement in extraction sites, partially or completely healed alveolar ridge situations
- Especially indicated for use in soft bone applications where implants with other implant surface treatments may be less effective
- Suitable for immediate loading* in all indications, except in single tooth situations in soft bone (type IV) where implant stability may be difficult to obtain and immediate loading may not be appropriate

***Immediate loading of single-tooth restoration is not recommended for OsseoSpeed™ TX Implant 4.0 S – 6 mm**

It is important that the clinician takes local loading conditions into consideration when determining the number and spacing of short implants. Considering the reduced bone support provided by short implants, it is important for the purpose of early diagnosis and treatment that the clinician closely monitor soft tissue and supporting bone health status by means of probing and radiographic evaluation when indicated.

From a mechanical strength point of view it is recommended to always place as wide implant as possible. This is particularly important in the posterior regions of the jaws where loading forces are high and considerable bending moments can be generated.

| OsseoSpeed™ TX Implant | 3.0 S  3.0 mm  1.7 mm | 3.5 S  3.5 mm  1.9 mm | 4.0 S  4.0 mm  2.4 mm | 4.5  4.5 mm  1.9 mm | 5.0  5.0 mm  2.4 mm | 5.0 S  5.0 mm  3.2 mm |
|------------------------|---|---|---|---|---|--|
| Indications | For replacement of maxillary laterals and mandibular central and lateral incisors when there is not enough space for a wider implant. | In all positions in the jaws. Single tooth to full arch. | In all positions in the jaws. Single tooth to full arch. | In all positions in the jaws. Single tooth to full arch. | In all positions in the jaws. Single tooth to full arch. | In all positions in the jaws. Especially indicated for wide ridges and large edentulous spaces and for increased stability in extraction sockets when doing immediate implant installation Single tooth to full arch. |
| Note | It is recommended that when possible, a wider implant should be used. | Single-standing, non-splinted restorations in the molar regions, should preferably be supported by wider implants. | OsseoSpeed™ TX 4.0 S implant – 6 mm should only be used when there is not enough space for a longer implant. Immediate loading in single tooth replacement is not recommended. | | | |

Drill overview

Implant sites are prepared in a step-by-step procedure using drills of different diameters to ensure an efficient and atraumatic widening of the implant site. All drilling of the bone tissue should be carried out under profuse external irrigation with saline solution and with an intermittent drilling technique to prevent heating of the bone and to create a pumping effect for efficient removal of bone tissue. All Astra Tech drills have laseretched depth indication lines that allow for distinct and clear depth reading.

Drills are available in two options:

Single Patient Drills

- Packaged sterile and opened as needed at time of surgery
- Optimized cutting properties and contamination-free ease of use
- Disposed after each surgery

Multiple-use Drills

- Optimal cutting properties
- Designed for multiple-use provided that they are carefully cleaned and sterilized after each surgery

Must be replaced as needed to ensure optimal cutting properties for each surgery.

Drill types

There are five basic drill types:



Guide Drill

To mark out and create the insertion point penetrating cortex to evaluate bone quantity and quality.




Twist Drill

To prepare the installation site, reaching final width and depth.



Pilot Drill

Optional drill to guide succeeding with twist drills, e.g. suitable to facilitate soft bone situation.



Cortical Drill

Drill for cervical preparation for OsseoSpeed™ TX 3.0 S, 3.5 S, 4.0 S and 5.0 S implants when the bone is dense. Used to enlarge the opening of an implant site to the exact implant diameter to reduce the pressure in the bone around the implant neck.




Conical Drill

The apical border of the indication line indicates the minimum depth needed to fit the implant. The recommendation is to drill to this depth in standard and soft bone situations. When the bone is dense the recommendation is to drill to the marginal border of the depth indication line. Make sure there is enough depth provided for the entire implant. Sometimes additional drilling with a twist drill is needed. Always make a check-up with the Implant Depth Gauge.


Drilling depth

The drilling depth is measured from the widest part of the drill tip up to the indication line. For Single Patient Drills, the additional depth is 0.9 mm regardless of drill diameter. For Multiple-use Drills, the additional depth or tip height created by the point of the drill is 0.6 to 1.45 mm, depending on the diameter and type of drill.

Single Patient Drills

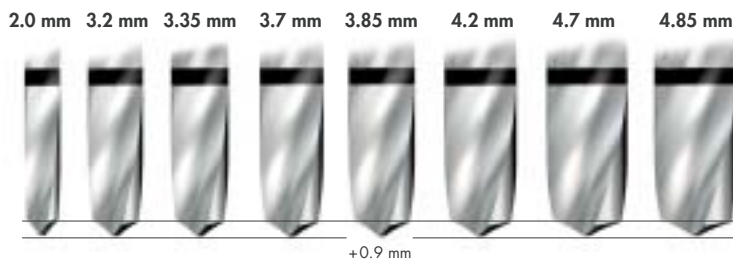

Multiple-use Drills

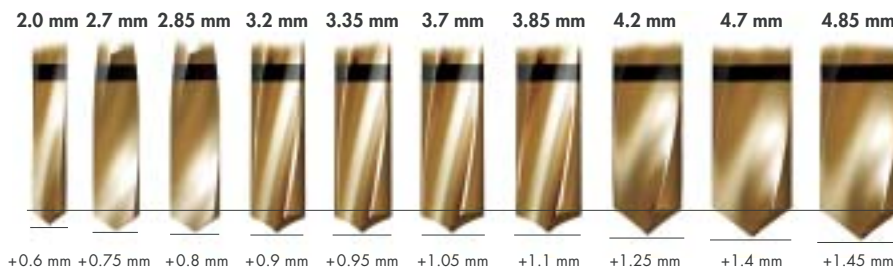

Twist Drill long, 8–19 mm



Twist Drill short, 8–13 mm



Twist Drill, 6–13 mm

Implant Depth Gauge

The depth indications on the Implant Depth Gauge correspond to the laser markings on the Twist Drills for the different implant lengths. A waist is available on the depth gauge to facilitate the identification of the 13–15 mm indication band. The lower part of the gauge has indications for 2–3, 4–5 mm and can be used for measuring soft tissue height.

When measuring the final prepared implant site, rest the depth gauge against the wall of the osteotomy.

Note: If the Implant Depth Gauge is placed in the deeper central part of the prepared implant site, the additional depth should be taken into account.



PREPARATION

Implant



Color-coding


For easy identification of the implant-abutment connection size the product packaging is color-coded:

- X-Small connection – Yellow: Implant diameter 3.0 mm
- Small connection – Aqua: Implant diameters 3.5 and 4.0 mm
- Large connection – Lilac: Implant diameters 4.5 and 5.0 mm



Peel off

Peel off the perforated section of the label and use it for documentation and/or communication with your restorative partner.

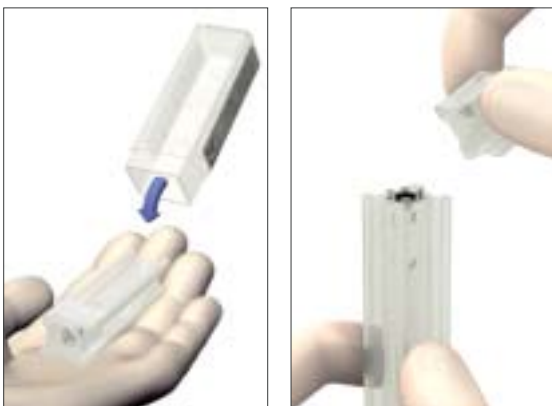

Open

Slide the sterile inner container onto a sterile surgical area. Lift the cap to expose the implant.



Pick up

Attach the appropriate Implant Driver to the Contra Angle.

Make sure that the driver is properly seated. Pick up the implant from the inner container.



Preparation of the Healing Abutment and Cover Screw

The Healing Abutment as well as the Cover Screw and other sterile abutments are packed in the same type of container as implants, with color-coded labels that indicate the implant-abutment connection size. They are mounted in a convenient plastic insert for direct access with a Hex Screwdriver.




Peel off and open

Peel off the perforated section of the label and use it for documentation and/or communication with your restorative partner. Open the container and slide the sterile inner insert onto a sterile surgical area.



Connect

Hold the inner insert steady and connect the Hex Screwdriver to the Healing Abutment or the Cover Screw with a friction fit.

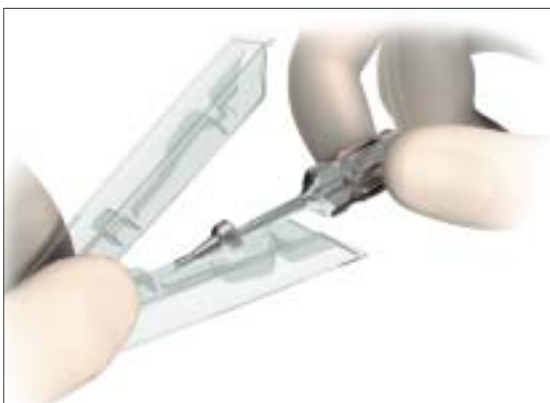


Lift out

Split the insert open and lift out the Healing Abutment or Cover Screw.

Surgical Tray and instruments

The Surgical Tray is designed to conveniently and easily manage the required drills, instruments, and implants for surgery. The layout of the tray navigates the surgeon through the drilling progression.

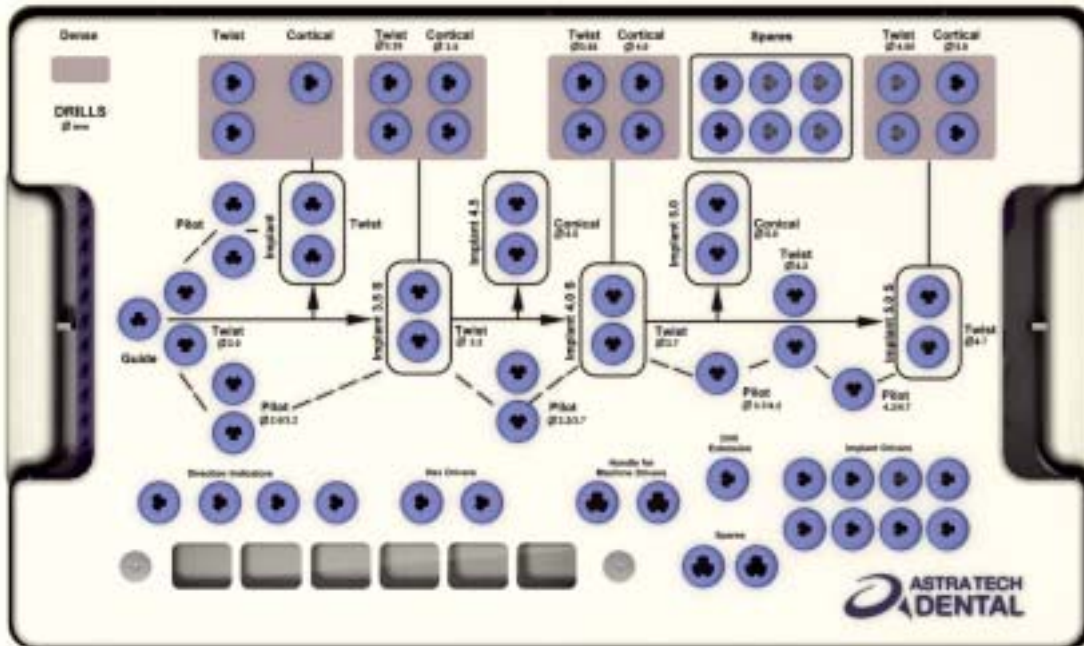

A complete line of instruments and drills needed for the surgical procedures are available.



Single Patient Drills provide the ideal surgical situation for each individual patient and give you the confidence of predictably sharp drills every time.

BoneTrap™ is the ideal collector for harvesting bone particles during surgery. The unique design of the filter allows for efficient collection of bone particles without clogging.

Cleaning and sterilization guidelines

Drills

Astra Tech provides Multiple-use and Single Patient Drills.

- Dispose of the Single Patient Drills into a sharps container immediately after the implant procedure is completed
- **Do not re-sterilize** the Single Patient Drills
- Reusable drills are designed to be cleaned, disinfected, placed back in the tray and sterilized after each use



Instruments, Multiple-use Drills and trays

Choose between the following two cleaning techniques

Cleaning technique 1:

- Clean Multiple-use Drills and instruments and then use an ultrasonic cleaner to ensure all the debris is removed. Rinse thoroughly



Cleaning technique 2:

- Clean and disinfect all Multiple-use Drills, instruments and trays within an instrument dishwasher

Sterilization

- Thoroughly dry Multiple-use Drills, instruments and trays before the sterilization process to prevent possible corrosion of the metal components
- Steam sterilize Multiple-use Drills, instruments and trays at 134°C/270-275°F for minimum 3 minutes (or corresponding method in accordance with autoclave manufacturers instruction)



Note: Ensure that both the Ratchet Wrench and/or combination Torque Wrench is dismantled before the cleaning and sterilization process.



Contra Angle

Choose between the following two cleaning techniques (please refer to manufacturer's instructions).

Cleaning technique 1:

- Disassemble the contra angle
- Clean with a soft brush under cold running water or in a dishwasher
- Thoroughly dry the contra angle
- Lubricate the contra angle according to the manufacturer's instruction

Cleaning technique 2:

- Clean and lubricate in an automatic unit for contra angles



Sterilization

- Steam sterilize the disassembled contra angle

References supporting the Astra Tech Implant System™

One- and two-stage surgery

Cecchinato D, Olsson C, Lindhe J. Submerged or non-submerged healing of endosseous implants to be used in the rehabilitation of partially dentate patients. *J Clin Periodontol* 2004;31(4):299-308. (ID No. 78302) [Abstract in PubMed](#)

Cecchinato D, Bengazi F, Blasi G, Botticelli D, Cardarelli I, Gualini F. Bone level alterations at implants placed in the posterior segments of the dentition: outcome of submerged/non-submerged healing. A 5-year multicenter, randomized, controlled clinical trial. *Clin Oral Implants Res* 2008;19(4):429-31. [Abstract in PubMed](#)

Geckili O, Bilhan H, Bilgin T. A 24-week prospective study comparing the stability of titanium dioxide grit-blasted dental implants with and without fluoride treatment. *Int J Oral Maxillofac Implants* 2009;24(4):684-8. (ID No. 79232) [Abstract in PubMed](#)

Cooper LF, Moriarty JD, Guckes AD, Klee LB, Smith RG, Almgren C, et al. Five-year prospective evaluation of mandibular overdentures retained by two microthreaded, TiOblast nonsplinted implants and retentive ball anchors. *Int J Oral Maxillofac Implants* 2008;23(4):696-704. [Abstract in PubMed](#)

Cooper LF, Ellner S, Moriarty J, Felton DA, Paquette D, Molina A, et al. Three-year evaluation of single-tooth implants restored 3 weeks after 1-stage surgery. *Int J Oral Maxillofac Implants* 2007;22(5):791-800. (ID No. 78988) [Abstract in PubMed](#)

Gotfredsen K. A 5-year prospective study of single-tooth replacements supported by the Astra Tech implant: a pilot study. *Clin Impl Dent Rel Res* 2004;6(1):1-8. (ID No. 78273) [Abstract in PubMed](#)

Vroom MG, Sipos P, de Lange GL, Grundemann LJ, Timmerman MF, Loos BG, et al. Effect of surface topography of screw-shaped titanium implants in humans on clinical and radiographic parameters: a 12-year prospective study. *Clin Oral Implants Res* 2009;20(11):1231-39. [Abstract in PubMed](#)

Wennström JL, Ekestubbe A, Gröndahl K, Karlsson S, Lindhe J. Oral rehabilitation with implant-supported fixed partial dentures in periodontitis-susceptible subjects. A 5-year prospective study. *J Clin Periodontol* 2004;31(9):713-24. (ID No. 78275) [Abstract in PubMed](#)

Yi SW, Ericsson I, Kim CK, Carlsson GE, Nilner K. Implant-supported fixed prostheses for the rehabilitation of periodontally compromised dentitions: a 3-year prospective clinical study. *Clin Impl Dent Rel Res* 2001;3(3):125-34. (ID No. 75415) [Abstract in PubMed](#)

Immediate placement/extraction sockets

Kahnberg KE. Immediate implant placement in fresh extraction sockets: a clinical report. *Int J Oral Maxillofac Implants* 2009;24(2):282-8. [Abstract in PubMed](#)

Cooper LF, Rahman A, Moriarty J, Chaffee N, Sacco D. Immediate mandibular rehabilitation with endosseous implants: simultaneous extraction, implant placement, and loading. *Int J Oral Maxillofac Implants* 2002;17(4):517-25. (ID No. 78110) [Abstract in PubMed](#)

Sanz M, Cecchinato D, Ferrus J, Pjetursson EB, Lang NP, Lindhe J. A prospective, randomized-controlled clinical trial to evaluate bone preservation using implants with different geometry placed into extraction sockets in the maxilla. *Clin Oral Implants Res* 2009;DOI: 10.1111/j.1600-0501.2009.01824.x. [Abstract in PubMed](#)

Lops D, Chiapasco M, Rossi A, Bressan E, Romeo E. Incidence of inter-proximal papilla between a tooth and an adjacent immediate implant placed into a fresh extraction socket: 1-year prospective study. *Clin Oral Implants Res* 2008;19(11):1135-40. (ID No. 79132) [Abstract in PubMed](#)

De Kok IJ, Chang SS, Moriarty JD, Cooper LF. A retrospective analysis of peri-implant tissue responses at immediate load/provisionalized microthreaded implants. *Int J Oral Maxillofac Implants* 2006;21(3):405-12. (ID No. 78727) [Abstract in PubMed](#)

Ferrus J, Cecchinato D, Pjetursson EB, Lang NP, Sanz M, Lindhe J. Factors influencing ridge alterations following immediate implant placement into extraction sockets. *Clin Oral Implants Res* 2009;DOI: 10.1111/j.1600-0501.2009.01825.x. [Abstract in PubMed](#)

Immediate and early loading

Collaert B, De Bruyn H. Early loading of four or five Astra Tech fixtures with a fixed cross-arch restoration in the mandible. *Clin Impl Dent Rel Res* 2002;4(3):133-5. (ID No. 78384) [Abstract in PubMed](#)

Steveling H, Roos J, Rasmusson L. Maxillary implants loaded at 3 months after insertion: results with Astra Tech implants after up to 5 years. *Clin Impl Dent Rel Res* 2001;3(3):120-4. (ID No. 75414) [Abstract in PubMed](#)

Oxby G, Lindqvist J, Nilsson P. Early loading of Astra Tech OsseoSpeed implants placed in thin alveolar ridges and fresh extraction sockets. *Appl Osseointegration Res* 2006;5:68-72. (ID No. 78735)

Cooper L, Felton DA, Kugelberg CF, Ellner S, Chaffee N, Molina AL, et al. A multicenter 12-month evaluation of single-tooth implants restored 3 weeks after 1-stage surgery. *Int J Oral Maxillofac Implants* 2001;16(2):182-92. (ID No. 75410) [Abstract in PubMed](#)

Collaert B, De Bruyn H. Immediate functional loading of TiOblast dental implants in full-arch edentulous maxillae: a 3-year prospective study. *Clin Oral Implants Res* 2008;19(12):1254-60. [Abstract in PubMed](#)

Donati M, La Scala V, Billi M, Di Dino B, Torrisi P, Berglundh T. Immediate functional loading of implants in single tooth replacement: a prospective clinical multicenter study. *Clin Oral Implants Res* 2008;19:740-48. (ID No. 79065) [Abstract in PubMed](#)

Toljanic JA, Baer RA, Ekstrand K, Thor A. Implant rehabilitation of the atrophic edentulous maxilla including immediate fixed provisional restoration without the use of bone grafting: a review of 1-year outcome data from a long-term prospective clinical trial. *Int J Oral Maxillofac Implants* 2009;24(3):518-26. [Abstract in PubMed](#)



$$A = \pi (r_1 \times S_1 - r_2 \times S)$$




Connective
Contour



Astra Tech BioManagement Complex™

A successful implant system cannot be determined by one single feature alone. Just as in nature, there must be several interdependent features working together. The following combination of key features is unique to the Astra Tech Implant System™:

- **OsseoSpeed™** — more bone more rapidly
- **MicroThread™** — biomechanical bone stimulation
- **Conical Seal Design™** — a strong and stable fit
- **Connective Contour™** — increased soft tissue contact zone and volume

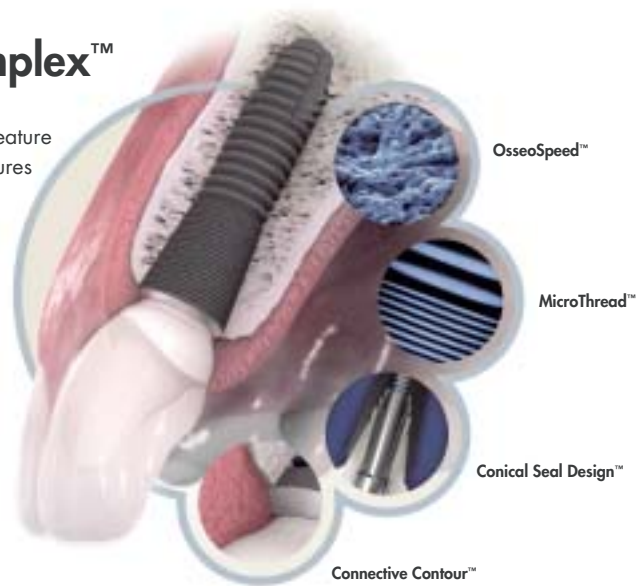

Australia

Astra Tech Pty Ltd.
Suite 1, 53 Grandview St, Pymble NSW 2073
☎ +61 2 9488 3500. ☎ +61 2 9440 0744
www.astratechdental.com.au

Austria

Astra Tech GesmbH
Schloßhofer Straße 4/4/19, AT-1210 Wien
☎ +43-(0)1-2146150. ☎ +43-(0)1-2146167
www.astratechdental.at

Benelux

Astra Tech Benelux B.V.
Signaalrood 55, NL-2718 SG Zoetermeer
☎ +31 79 360 1955/+32 3 232 81 50
☎ +31 79 362 3748/+32 3 213 30 66
www.astratechdental.nl

Canada

Astra Tech Inc.
2425 Matheson Blvd East, 8th Floor
Mississauga, ON L4W 5K4
☎ +1 905 361 2844
www.astratechdental.com

Denmark

Astra Tech A/S
Roskildevej 163, 1. th., DK-2620 Albertslund
☎ +45 43 71 33 77. ☎ +45 43 71 78 65
www.astratechdental.dk

East Asia

Astra Tech
Suite 15.02, 15th Floor Menara PanGlobal
No. 8 Lorong P Ramlee, MY-50250, Kuala Lumpur
Malaysia
☎ +60 3 27 11 2531. ☎ +60 3 27 11 2532
www.astratechdental.com

Finland

Astra Tech Oy
PL 96, FI-02231 Espoo
☎ +358 9 8676 1626. ☎ +358 9 804 4128
www.astratechdental.fi

France

Astra Tech France
7, rue Eugène et Armand Peugeot, TSA 90002
FR-92563 Rueil Malmaison Cedex
☎ +33 1 41 39 02 40. ☎ +33 1 41 39 02 44
www.astratechdental.fr

Germany

Astra Tech GmbH
An der kleinen Seite 8. DE-65604 Elz
☎ +49 6431 9869 0. ☎ +49 6431 9869 500
www.astratechdental.de

Italy

Astra Tech S.p.A.
Via Cristoni, 86, IT-40033 Casalecchio di Reno (BO)
☎ +39 051 29 87 511. ☎ +39 051 29 87 580
www.astratechdental.it

Japan

Astra Tech K.K.
1-7-16 Sendagaya, Shibuya-ku, Tokyo 151-0051
☎ +81 3 5775 0515. ☎ +81 3 5775 0571
www.astratech.jp

Norway

Astra Tech AS
Postboks 160, NO-1471 Lørenskog
☎ +47 67 92 05 50. ☎ +47 67 92 05 60
www.astratechdental.no

Poland

Astra Tech Sp. z o.o.
ul. Oreżna 58, PL-02-937 Warszawa
☎ +48 22 853 67 06. ☎ +48 22 853 67 10
www.astratechdental.pl

Portugal

Astra Tech
Lagoas Park, Edifício 8 – 1º piso
PT-2740-268 Porto Salvo
☎ +351 21 421 2273. ☎ +351 21 421 0234
www.astratechdental.pt

Spain

Astra Tech S.A.
Calle Ciencias nº 73 derecha. Nave 9,
Polígono Industrial Pedrosa,
ES-08908 L'Hospitalet de Llobregat
☎ Servicio al cliente: +34.902.101.558
☎ +34.932.643.560. ☎ +34.933.363.231
www.astratechdental.es

Sweden

Astra Tech AB
P.O. Box 14, SE-431 21 Mölndal
☎ +46 31 776 30 00. ☎ +46 31 776 30 17
www.astratechdental.se

Switzerland

Astra Tech SA
Avenue de Sévelin 18, P.O. Box 54
CH-1000 Lausanne 20
☎ +41 21 620 02 30. ☎ +41 21 620 02 31
www.astratechdental.ch

United Kingdom

Astra Tech Ltd.
Brunel Way, Stonehouse, Glos GL10 3SX
☎ +44 1453 791763. ☎ +44 1453 791001
www.astratechdental.co.uk

USA

Astra Tech Inc.
590 Lincoln Street, Waltham, MA 02451
☎ +1-800-531-3481. ☎ +1-781-890-6808
www.astratechdental.com

Other Markets

Astra Tech AB, Export Department
P.O. Box 14, SE-431 21 Mölndal, Sweden
☎ +46 31 776 30 00. ☎ +46 31 776 30 23
www.astratechdental.com

